



At the Forefront of Elite MSK Ultrasound with the Aplio i800 / Prism Edition

Aaron Fleming is a Senior Sonographer at Qscan Radiology's Red Hill Clinic in Brisbane, Australia – a leading diagnostic medical imaging and interventional practice that provides the imaging for numerous professional sporting teams and organizations as well as the general public. Aaron has a particular interest in MSK ultrasound that has evolved from an unparalleled passion for sport – a product of his upbringing in country NSW. One of the first specialists to scan with the new Aplio i-series / Prism Edition ultrasound system from Canon Medical, Aaron explained to VISIONS how the advanced new features and improved ergonomics enhance the scanning experience and facilitate greater accuracy in ultrasound diagnoses.

Striking additions

Aaron presented on his initial experiences of the Aplio i-series / Prism Edition at its global launch at the 2021 Australasian Sonographers Association (ASA) Conference in Brisbane, Australia, as well as at the Singapore Radiological Society and College of Radiologists.

“Scanning with the Aplio i800 / Prism Edition was a fantastic experience,” he remarked. “First and foremost, the image quality is the main strength. It allows

improved visualization of anatomy and pathology and, therefore, improved diagnostic accuracy.

Some of the cases scanned and images obtained during my experience with the machine are testament to the quality of the system."

In addition, there are a number of really smart new features that improve the overall scanning experience. Some highly advanced new technologies, the customizable control panel and interface, the electric lift button and the increased versatility of the transducers were all striking additions to the new Aplio i-series / Prism Edition.

iBeam+ technology on the new Aplio i-series / Prism Edition emits, receives and processes ultrasound with up to four times faster image processing. The improved bandwidth and processing power of the iBeam+ beamformer results in images with better penetration and detail resolution, so more can be seen without having to switch to a lower frequency transducer.

Aplio's innovative Full Focus function enables clear, uniform images from near to far field without the need for tedious focus adjustments. With fewer application steps and greater uniformity, this can be particularly useful for a number of examinations.

Next-generation Superb Micro-vascular Imaging (SMI) capability on the Prism Edition is further enhanced to provide a higher frame rate, leading to better visualization and less clutter. Doppler luminance also produces an aesthetically pleasing image.

Advantages of the Prism Edition for MSK

'From an MSK point of view, I think this system can help challenge and even overturn the notion that MRI is the gold standard for MSK imaging,' Aaron says. Ultrasound offers many benefits over MRI such as availability, cost and superior spatial resolution to name

but a few. Tendon and especially nerve assessment with ultrasound can trump MRI. Furthermore, ultrasound can be used for screening checks and in the rehab and progress of various injuries providing invaluable prognostic information and up-to-date return to play estimates for the team that oversees the care and treatment of professional and amateur athletes.

"There are a number of new, really smart features that improve image quality as well as the scanning experience."

Versatile transducers

"The Prism Edition's transducers are very versatile. The matrix probes all produced fantastic images and you could have quite easily performed the same scan with a number of different probes with no loss in scanning confidence."

For Clinical Case 1 – Aaron used a High Frequency 24 MHz (i24LX8) linear matrix transducer, to demonstrate an intact Flexor Digitorum Profundus (FDP) and Flexor Digitorum Superficialis (FDS) tendons of the second finger. However, there were changes to the echogenicity of the adjacent lumbrical muscle. The muscle appeared enlarged and heterogeneous with anechoic areas consistent with fluid. Increased vascularity was detected with SMI using Doppler luminance. These findings are consistent with a partial tear of the first lumbrical muscle of the hand – an unusual occurrence.



Scan the QR-code or click here to view the presentation

Qscan

Qscan Radiology Clinics is a comprehensive Diagnostic Medical Imaging & Interventional practice with subspecialty trained Radiologists, and highly trained clinical and support staff across multiple clinics in South-East Queensland and additional Qscan Group partner clinics elsewhere in Australia.

Qscan Radiology has a team of Radiologists who are highly experienced in sport imaging.
<https://www.qscan.com.au>

In another case, Clinical Case 3, the Aplio i800 / Prism Edition's 22 MHz High Frequency Hockey Stick transducer (i22LH8) was used to scan the thumb of an elite AFLW player – whose thumb was injured in a contest. A full thickness tear of the RCL and an avulsion fracture of the first metacarpal joint were visualized. Ultrasound findings also suggested a partial thickness tear of the UCL with no Stener lesion.

Canon Medical provides two high-frequency hockey sticks from 17 to 22 MHz with the Aplio i800 / Prism Edition. Both hockey sticks have a very fine footprint that allows easy access for imaging superficial areas in hard-to-reach anatomical places. 'The interventional radiologists were also big fans of the hockey stick transducers.'

Better ergonomics

Ergonomics are an important aspect of scanning for any sonographer.

Aaron found that the electric lift button as a sit/stand sonographer improved this aspect tremendously.

“New, highly advanced technologies, the customizable control panel and interface, the electric lift button are all striking features to the versatility of the Aplio i-series / Prism Edition.”



Biography

Aaron Fleming is a Senior Sonographer at Qscan Radiology Red Hill Clinic, in Queensland, Australia – a leading diagnostic medical imaging and interventional practice with a high level of expertise in sport imaging. Aaron has a particular interest in MSK that has evolved from his passion for sport.

He graduated from radiography at Newcastle University in 2009 and completed a post-graduate diploma in Medical Ultrasound at Queensland University of Technology (QUT), Brisbane, Australia, in 2013.

He also found the Aplio i800 / Prism Edition was very customizable which added benefits not just to ergonomics but in flattening the learning curve inherent in adjusting to a new machine.

“Similar to previous models, you have control over the setup of the control panel and interface. Therefore, there is next to no lag time in adjusting to a new machine,” he said. “Furthermore, the additions to previous models are all very intuitive, so it was very easy-to-use, and the learning curve was very smooth.”

Vast possibilities

With some prior knowledge of the Aplio i-series, Aaron was not really surprised by the image quality of the latest Aplio i800 / Prism Edition, however he was impressed with the further improvements to the already strong features of previous Aplio systems.

“It’s exciting to think of where this could lead,” he said. “The potential possibilities are vast and really positive for ultrasound. Some of the AI components of the new Aplio

system are a really exciting prospect. I didn’t get to use a lot of these in this instance, but AI is something that I think sonographers and radiology should really embrace.” //



Scan the QR code or click [HERE](#) to watch Canon Medical's video about the Aplio i-series / Prism Edition!

Case 2: Distal Biceps Tear

This case study follows a 52-year-old firefighter who presented to his doctor with pain in his left elbow upon pronation and supination. There was no acute injury reported by the patient. Possible distal biceps tendinosis was thought to be the cause of his symptoms.

The scan revealed a high-grade partial tear of the distal biceps at its insertion, predominantly involving the long head of biceps. Some vascularity in the distal biceps was also demonstrated with Superb Microvascular Imaging (SMI). Post diagnosis, it was recommended that the patient return for a Platelet Rich Plasma (PRP) injection into the area to help with tendon repair and alleviate symptoms.

Partial tear findings of the long head of biceps are an important diagnosis to help prevent the possibility of further full thickness tearing. The deep section of the distal insertion of biceps can be difficult to image.

** Ultrasound examination was performed using the versatile 18 to 5 MHz (i18LX5) intelligent Dynamic MicroSlice (iDMS) transducer able to cover all joints and MSK structures from skin to bone.*

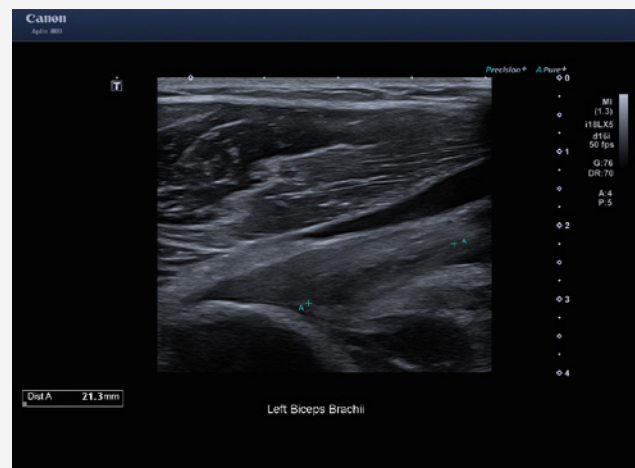


Figure 1: The biceps can be seen at its distal insertion onto the radial tuberosity. The deep portion of the tendon is seen to be heterogenous over an area of 21mm thought to be consistent with a partial tear of this tendon.

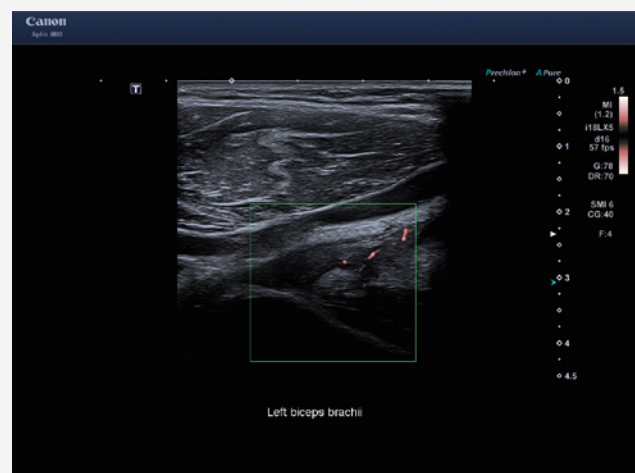


Figure 2: SMI shows some increased hyperaemia in the region of interest.

Case 3: Radial Collateral Ligament Tear

A 29-year-old female AFL player presented with pain in the first metacarpophalangeal joint (MCP) following a hyper-extension injury.

A full thickness tear of the radial collateral ligament (RCL) and an avulsion fracture of the first metacarpal joint were visualised. Ultrasound findings also suggested a partial thickness tear of the ulnar collateral ligament (UCL) without a Stener Lesion.

The ulnar and radial collateral ligaments are the two main supporting structures that traverse the metacarpophalangeal (MCP) joint of the thumb. Forced adduction is the most common cause of injury to the RCL, while forced abduction movements are the cause of most acute injuries to the UCL. The damage sustained to both ligaments were clearly demonstrated in this hyperflexion case.

* An ultrasound examination was performed using a 22 MHz High Frequency Hockey Stick transducer (i22LH8) with very fine footprint allowing easy access for imaging superficial areas in hard-to-reach anatomical places.

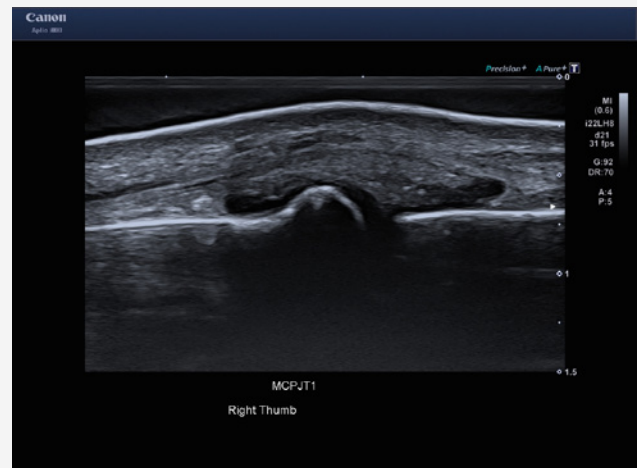


Figure 1: Imaging of the MCP Joint clearly demonstrates fluid emanating from the joint.

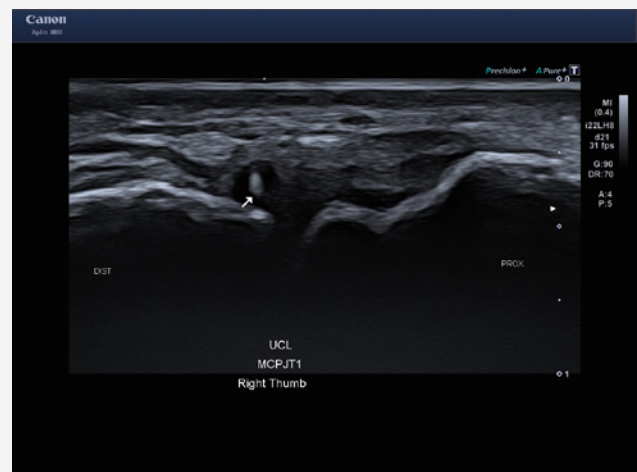


Figure 2: Imaging of the UCL shows an echogenic area at the distal portion of the ligament. Findings are suggestive of a partial tear.

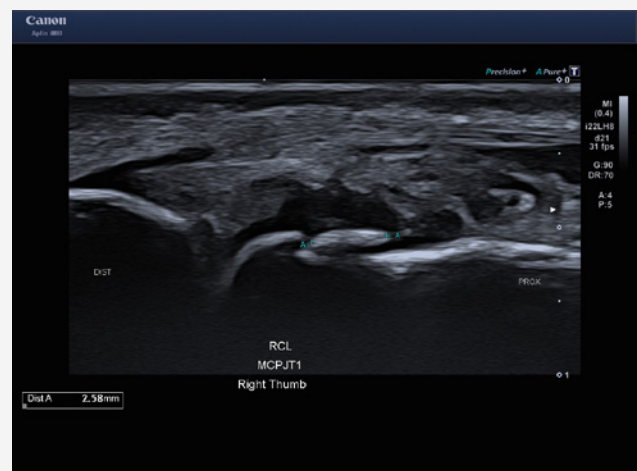


Figure 3: Imaging of the RCL of the thumb shows a 2.5mm echogenic area at the proximal portion of the ligament suggestive of an avulsion fracture.